

The mathematical model of rainwater catchment in Wrocław

Monika Nowakowska^{1,*}

¹Faculty of Environmental Engineering, Wrocław University of Science and Technology, Department of Water and Sewage, Wybrzeże Wyspiańskiego 27, 50-370 Wrocław, Poland

Abstract. On the basis of field studies of canalized storm water catchment of Gaj and Tarnogaj estate in Wrocław the rules of construction of hydrodynamic models in SWMM program were presented. The process of identification of hydrological and hydraulic parameters of the model, in the course of its calibration and validation were presented. To assess the quality of model the rates and statistical criteria were proposed to compare the results of stream simulation and volume of runoff of effective precipitation with the results of the measurements.

1 Introduction

Escalating in recent years extreme weather phenomena such as incidental or prolonged rainfall and associated with them flooding cause significant economic losses. In the existing, modernized or newly designed sewage systems the verification of hydraulic capacity of networks and objects is now recommended, including overflows from channels towards hydrodynamic modeling at different scenarios of precipitation load.

Modeling of systems reliability recommended by standard PN-EN 752:2008 is rarely applied in Poland [1] – with regard to the verification of the frequency of overflow from channels and even required by law according to the regulation of the Minister of the environment from 2014 [2] – with regard to the verification of the frequency of storm water overflows. This is mainly the result of the lack of sufficient basis of modeling methods as well as appropriate output databases with regard to monitoring of precipitation and overflows in sewage systems [3]. For instance, the level of integration of sub-catchment area is as yet intuitively. Usually channels with diameter smaller than 0.5 m are omitted and the width of the hydraulic sub-catchment is designated from several different formulas. In calibration and validation of hydrodynamic models data from the short period of observation are taken into consideration (i.e. few months) and the assessment of the quality of hydrodynamic models is based on various statistical indicators for comparison of the simulation results of sewage with the measurement results.

Based on the example of local data regarding the precipitation and streams of storm water in Wrocław the principles of the construction of mathematical model for drainage the area in SWMM program were presented.

* Corresponding author: monika.nowakowska@pwr.edu.pl

2 Material and methods of studies

For field research the canalized catchment of Gaj and Tarnogaj estate in Wrocław were selected, with the area $F = 104$ hectares – giving runoff to indoor drainage collector KD1 (with diameters from 0.3 m to 1.4 m). From the total area of estates, the dimpled areas were excluded, including allotments from which the sewage runoff of precipitation taking place into the ditches. The total length of the inventoried channels was 17731 m and the number of drains 509. This gives an average spacing of drains 34.8 m, which can be considered as representative for the cities.

On the stage of identification, as a minimum diameter of channels taking $d_{min} \geq 0.3$ m, 75 catchment area were discharged. In sub-catchments sealed areas were distinguished – not having retention F_d (roofs), sealed areas-with retention F_a (asphalt road) and $F_{k,b}$ (carriageways with concrete block or cobblestone) and areas not sealed ("green" areas) – with retention F_{nu} . Then degrees of sealed area were calculated in each sub-catchments: total sealing degree: $\%F_u = F_u/F_i$, degree of area sealing without retention: $\%F_{ubr} = F_{ubr}/F_u$ and degree of area sealing with retention: $\%F_{uzr} = F_{uzr}/F_u$. Slope of area (i_p) in the sub-catchments were adopted as weighted average-from the area of the terrain, streets, squares and roofs (tab. 1).

Table 1. Summary of characteristic area and slope of sub-catchments.

Area no.	Mark of catchment area	Node no.	Catchment area F_i	Sealed areas F_u				Areas not sealed F_{nu}	$\%F_u$	$\%F_{ubr}$	$\%F_{uzr}$	i_p
				F_d	F_a	F_b	ΣF_u					
				ha								
1	P1	18	09019	0.1175	0.1926	0.3315	0.6416	0.2603	71.1	18.3	81.7	1.20
4	P4	45	13590	0.6212	0.0000	0.7378	1.3590	0.0000	100.0	45.7	54.3	1.18
9	P9	65	02985	0.0000	0.1178	0.0407	0.1585	0.1400	53.1	0.0	100.0	1.11
12	P11	73	24492	0.6616	1.3501	0.0858	2.0974	0.3517	85.6	31.5	68.5	1.21
16	P14.1	119	02220	0.0000	0.0929	0.0260	0.1189	0.1031	53.6	0.0	100.0	1.12
20	P16.1	99	34074	1.2146	0.2309	1.5695	3.0150	0.3924	88.5	40.3	59.7	1.10
21	P17	121	05730	0.0000	0.1896	0.1891	0.3787	0.1943	66.1	0.0	100.0	0.17
31	P21.1	142	1.0254	0.0000	0.8203	0.1230	0.9434	0.0820	92.0	0.0	100.0	0.33
32	P22	170	2.2621	0.1900	0.0414	0.1015	0.3330	1.9291	14.7	57.1	42.9	0.22
33	P23	170	1.8855	0.0000	0.2625	0.3150	0.5775	1.3080	30.6	0.0	100.0	0.68
34	P24	182	3.4543	0.4098	0.0609	0.0895	0.5602	2.8941	16.2	73.2	26.8	0.18
37	P26	242	0.6718	0.0000	0.1671	0.1537	0.3208	0.3510	47.8	0.0	100.0	1.01
43	P28.2	238.0	1.3525	0.3852	0.0000	0.0553	0.4405	0.9120	32.6	87.4	12.6	0.72
56	P38	322	0.7092	0.0263	0.4255	0.2128	0.6646	0.0446	93.7	4.0	96.0	1.81
68	P46	382	5.3379	1.3345	0.4404	0.8195	2.5944	2.7435	48.6	51.4	48.6	0.55
71	P48	454	0.5189	0.0000	0.1920	0.0327	0.2247	0.2942	43.3	0.0	100.0	0.92
75	P51	505	1.0265	0.1721	0.2344	0.1875	0.5940	0.4325	57.9	29.0	71.0	1.20
SUM/AVERAGE			103.98	23.66	15.41	22.44	61.50	42.47	59.2	38.5	61.5	0.93
MIN			0.2220	0.0000	0.0000	0.0260	0.1189	0.0000	14.7	0.0	12.6	0.17
MAX			5.3379	1.3345	1.3501	1.5695	3.0150	2.8941	100	87.4	100	1.81

Individual sub-catchments were organized into 75 network nodes, to which rainwater is drained (fig. 1).



Fig. 1. The scheme of the analyzed storm water drainage in SWMM program.

As the basis to determine hydraulic width of sub-catchment (W), the basic form of the formula was taken:

$$W = x\sqrt{F} \tag{1}$$

where:

F – area of storm water catchment/sub-catchment, m².

In subject literature, the formula (1) is most commonly used with multipliers for values: $x = 1.0$ [6–8] or $x = 1.5$ [9–11]. In Wrocław's conditions to render the parameter W it turned out that the best value was $x = 1.6$, which will be demonstrated later in this study.

To conduct simulation calculations in SWMM program it was necessary to create databases involving precipitation of rain in catchment and measurement of sewage streams in KD1 collector. For metering sewage streams two ultrasonic flow meters were used. Nivus type flow meter (P1 – fig. 1) was installed in drain no. 18 on the section of KD1 with a diameter of 1.4 m. The second type of flow meter Teledyne (P2) was installed in the drain no. 239, on the section KD1 with a diameter of 1.2 m.

The rain gauge type TRwS was a device used to register rainfall in the catchment located on the southern boundary of the catchment area of Gaj and Tarnogaj estate at a distance of about 620 m from the center of gravity of the tested catchment (fig. 1). Registry of precipitation was conducted for a period of 2 years, from July 29th 2013 to July 19th 2015. Precipitation with duration time $t > 45$ min and height $h > 10$ mm were taken for calibration and validation of the model. Both torrential rains - those of short duration (convective K), as well as those of long-term (frontal F and lowland N), which hyetographs have a continuous character were taken into consideration. The chosen precipitation was assigned later to their frequency of occurrence in Wrocław. As a criterion to determine the frequency of precipitation occurrence was taken the probabilistic model of maximum height in Wrocław (based on the distribution of Fisher-Tippett type III) – for $C \in [1; 100]$ years [12], and for precipitation occurring more frequently than once a year ($C \in [0.1; 1]$) a physical model was used [3]. These precipitations were detailed about episodes of time duration equal to time of flow of sewage in collector KD1 to the intersection of flowmeter P1 ($t \approx 45$ min) and P2 ($t \approx 15$ min). The parameters of 8 precipitation selected for calibration and validation of the model are given in table 2.

Table 2. The parameters of precipitation for calibration (no. 1–5) and validation of model (no. 6–8).

Number, type and date of precipitation	Time		Time <i>t</i> min	Σh mm	<i>C</i> year s	<i>h</i> ₄₅ mm	<i>C</i> ₄₅ years	<i>h</i> ₁₅ mm	<i>C</i> ₁₅ years
	from	to							
1. F 17.05.2014	09:45	17:09	444	15.1	0.55	5.6	0.36	3.0	0.27
2. N 23–24.07.2014	23:34	15:09	935	13.1	0.41	3.4	0.19	1.7	0.13
3. N 1–2.09.2014	15:27	13:47	1340	13.4	0.40	1.7	<0.1	1.0	<0.1
4. N 11.09.2014	8:01	22:54	894	11.7	0.38	2.4	0.12	1.6	0.11
5. N 22–23.10.2014	01:00	01:28	1468	28.4	0.75	2.2	0.11	1.5	0.11
6. K 29.07.2013	20:26	22:12	106	15.7	0.85	14.6	1.1	13.4	2.4
7. K 17.10.2014	18:37	20:12	95	9.7	0.52	8.6	0.59	6.1	0.61
8. K 19.07.2015	19:57	20:39	42	23.8	5.1	23.8	4.7	22.1	18.4

To assess the quality of the model selected statistical measure were used for comparing the results of measurements and calculations of the outflow (*Q*), such as [3–5, 13–15]:

- special rate of correlation *RS*:

$$RS = \sqrt{\frac{\sum_{i=1}^n (2 \cdot Q_{p,i} \cdot Q_{o,i} - Q_{o,i}^2)}{\sum_{i=1}^n Q_{p,i}^2}} \quad (2)$$

- relative residual error *WBR*:

$$WBR = \sqrt{\frac{n \cdot (\sum_{i=1}^n (Q_{p,i} - Q_{o,i})^2)}{\sum Q_{p,i}}} \quad (3)$$

- average value error *SWS*:

$$SWS = \bar{Q}_o / \bar{Q}_p \quad (4)$$

- relative error of maximum streams ΔQ_{max} :

$$\Delta Q_{max} = \frac{Q_{max,p} - Q_{max,o}}{Q_{max,p}} \cdot 100\% \quad (5)$$

Indexes "p", and "o" in formulas (2–5) mean respectively measurements and calculations. The value "n" corresponds to the number of extracted compartments-averaged values *Q* in a registered hydrographic of runoff. Depending on the value of the rate, the model can be qualified for the specified category. Ranges of values of rates *RS* and *WBR* together with corresponding categories of models were listed in table 3. For *SWS* rates and ΔQ_{max} the ranges of values for the appropriate category of model were not specified. The only known limit values appropriate for situation when the model perfectly reproduces reality: *SWS* = 1.0 i ΔQ_{max} = 0.

Table 3. Categories for the classification of the models.

Category of model	Rates-ranges of values	
	RS [-]	WBR [%]
Excellent	1.00–0.99	0–3
Very good	0.99–0.95	3–6
Good	0.95–0.90	6–10
Average	0.90–0.85	10–25
Dissatisfying	< 0.85	> 25

3 Calibration of model

Calibration of hydrodynamic model was based on determining the values of parameters:

- hydraulic – roughness rate of channels (n - to Manning formula) and roughness rate of sealed (n_{pu}) and unsealed (n_{pmu}) catchment areas,
- hydrological – the height of retention on sealed (h_{pu}) and unsealed (h_{pmu}) catchment areas.

Hydrogeological parameters of model (infiltration) were estimated by model of expert. As a result of the simulation calculations in SWMM program for 5 long-term precipitation calibration (type F and N-table 2) the empirical parameters of the model were determined. In table 4 the literature (output) and resulting values of the parameters of model of the tested drainage system were listed.

Table 4. The value of the calibration parameters of the model of tested drainage system.

Parameter	The width of the hydraulic sub-catchment	Rate of roughness - channels	Rate of roughness -sealed area	Rate of roughness -unsealed area	Height retention -sealed area	Height retention -unsealed area	The initial intensity infiltration-	Final intensity of infiltration- Horton's model	Constant recession -Horton's model	Lad drying time- Horton
Symbol	W	n	n_{pu}	n_{pmu}	h_{pu}	h_{pmu}	I_{in0}	I_{ink}	r	T_s
Unit	m	s/m ^{1/3}	s/m ^{1/3}	s/m ^{1/3}	mm	mm	mm/h	mm/h	h ⁻¹	d
Literature data for calibration	various formulas	0.013–0.020	0.011–0.050	0.1–0.8	1.3–2.5	2.5–7.5	8–254	0.2–20	2–7	2–14
Results of model's calibration in SWMM program	$1.6\sqrt{F}$	0.020	0.020	0.3	2.0	5.0	90	10	4	7

About the optimum values of parameters of the model proclaim the achieved values of indicators: RS, WBR, SWS and ΔQ_{max} , adopted as the statistical criteria to evaluate the quality of the model. However, the most important was the achievement of the compliance of simulated values with the values measured with respect to the balance of the volume of runoff (V), as shown in Chapter 4. In table 5 the final results of the calculation accuracy of the model for 5 precipitation calibrations and three forms of formula for the parameter W . The best results were achieved for $W3$. On the basis of the value of the indicators RS and WBR the calibrated model was assessed on the border of grades good and very good (according to the criteria from the table 3).

Figure 2 shows, for example, a histogram of precipitation and hydrographs of sewage streams in collector KD1 (intersection P1) for the latest lowland precipitation (N) from October 22nd to 23rd 2014.

Table 5. The results of the calculations of the calibration model.

Formula	Precipitation data FLOWMETER	17.05.2014		23-24.07.2014		1-2.09.2014		11.09.2014		22-23.10.2014	
		P1	P2	P1	P2	P1	P2	P1	P2	P1	P2
$W1 = \sqrt{F}$	RS [-]	0.977	0.930	0.977	0.970	0.967	0.973	0.958	0.938	0.980	0.976
	WBR [%]	4.0	7.3	5.9	7.2	6.0	5.9	6.8	9.8	4.7	5.2
	SWS [-]	0.940	1.030	0.989	1.113	0.993	1.011	1.057	1.147	1.018	1.100
	ΔQ_{max} [%]	14.9	20.8	0.9	-6.4	9.8	0.9	18.2	13.7	16.5	12.3
$W2 = 1.5\sqrt{F}$	RS [-]	0.985	0.949	0.983	0.970	0.971	0.976	0.968	0.954	0.982	0.978
	WBR [%]	3.2	6.2	5.1	7.2	5.6	5.4	6.0	8.5	4.5	5.0
	SWS [-]	0.943	1.032	0.993	1.117	0.997	1.014	1.061	1.150	1.019	1.099
	ΔQ_{max} [%]	11.5	14.5	-0.4	-10.6	6.9	-6.3	14.5	7.1	16.1	11.8
$W3 = 1.6\sqrt{F}$	RS [-]	0.986	0.951	0.983	0.970	0.972	0.977	0.969	0.956	0.982	0.979
	WBR [%]	3.1	6.1	5.0	7.3	5.6	5.4	5.9	8.3	4.4	5.0
	SWS [-]	0.943	1.033	0.994	1.117	0.997	1.014	1.061	1.151	1.020	1.099
	ΔQ_{max} [%]	11.0	13.6	-0.6	-11.2	6.5	-7.4	14.0	6.3	16.0	11.7

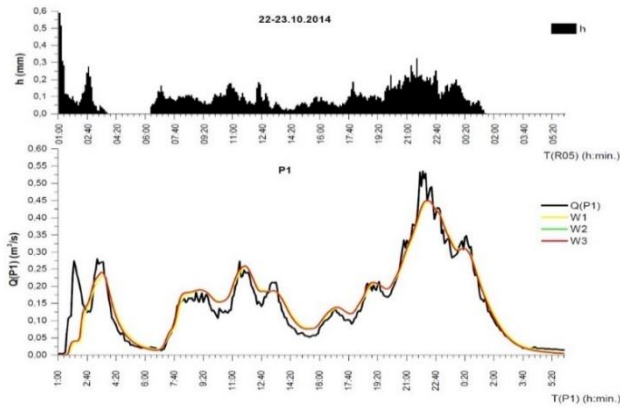


Fig. 2. A histogram of precipitation and hydrographs of flow into the collector KD1 (P1) for the latest lowland precipitation from October 22nd to 23rd 2014.

4 Validation of model

Validation of tested hydrodynamic model of drainage system consists in checking the accuracy of the already calibrated model on the 3 short-lived intense convective precipitation (K-tab. 2) with criterion of compatibility of the balance volume of runoff (V). Figure 3 shows an example of histogram of convective precipitation from July 19th 2015 and hydrographs of drainage (measured and simulated) in collector KD1 in the intersection of flowmeter P1.

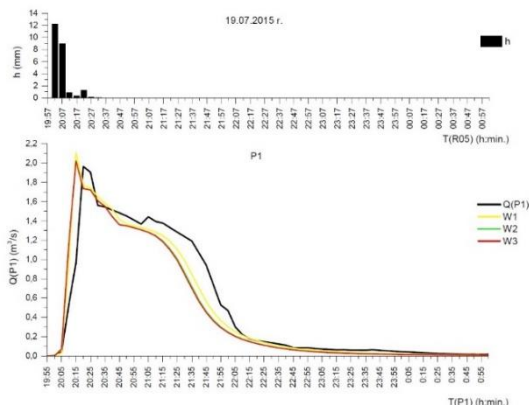


Fig. 3. A histogram of precipitation and hydrographs of flow into the collector KD1 (P1) – for convective precipitation from July 19th 2015.

Table 6 presents the results of a calculation parameter W for 3 validated precipitation (K). Accuracy of mapping of tested phenomena precipitation-outflow through the created model of canalized storm water catchment were presented cumulatively for 8 precipitation, i.e. 5 from calibration and 3 from validation. Figure 4 shows the correspondence with the volume balance of runoff (V).

Table 6. The results of the validation calculations.

Formula	Precipitation data /flowmeter	29.07.2013	17.10.2014		19.07.2015
		P1	P1	P2	P1
$W1 = \sqrt{F}$	RS [-]	0.988	0.994	0.992	0.970
	WBR [%]	2.2	1.1	1.6	3.0
	SWS [-]	1.122	1.070	1.089	0.932
	ΔQ_{max} [%]	-3.0	3.3	5.4	-7.2
$W2 = 1.5\sqrt{F}$	RS [-]	0.978	0.996	0.995	0.962
	WBR [%]	3.0	0.9	1.2	3.3
	SWS [-]	1.098	1.083	1.102	0.883
	ΔQ_{max} [%]	-7.7	-0.3	-0.8	-3.2
$W3 = 1.6\sqrt{F}$	RS [-]	0.978	0.996	0.995	0.961
	WBR [%]	3.0	1.0	1.3	3.4
	SWS [-]	1.090	1.084	1.103	0.876
	ΔQ_{max} [%]	-5.5	-1.0	-1.7	-2.8

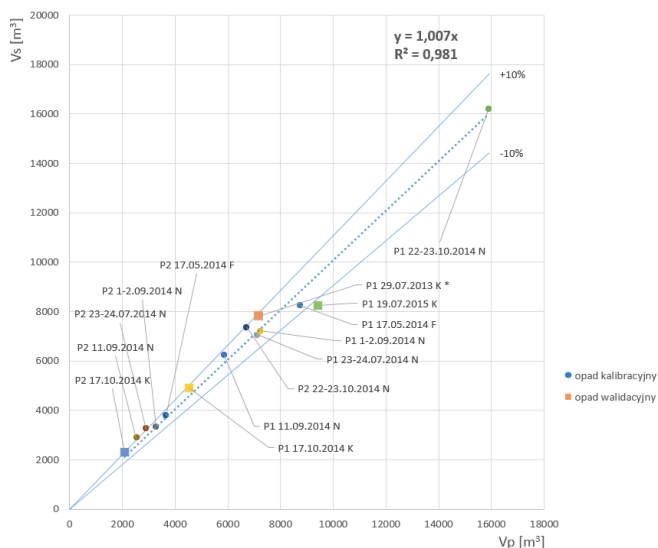


Fig. 4. The volume balance of runoff for precipitation from calibration and validation model.

Figure 4 shows that for 8 precipitations (from calibration and validation model) the volume of runoff describes the simple equation $V_s \approx V_p$ where $R^2 = 0.981$. This means high compliance of the simulated (S) and measured (P) volumes of precipitations runoff – 14 results of measurements and simulation is in the range accuracy $\pm 10\%$.

5 Summary and conclusions

In this paper the rules for the mathematical model of the drainage system in Wrocław area in SWMM program were showed. Selected results of studies about identification, calibration and validation of empirical parameters of the model along with the verification of formulas to determine the width of the hydraulic (W) sub-catchment were presented. Discussed results of this study have in methodical part universal character and are used to build models of other hydrodynamic urban catchment. Identification of the major parameters of empirical models (n , n_{pu} , n_{pmu} , h_{pu} and h_{pmu}) should be carried out in the course of their calibration on long-term precipitation (frontal and lowland) and in the course of the validation of the models on the intense precipitation (convection) with the compatibility criterion of the balance volume of runoff (V). To assess the quality of models the optional statistical indicators can be used (RS, WBR, SWS and ΔQ_{max}) describing the fitting accuracy of simulated and measured values of waste water streams.

The work was realized within the allocation No. 0401/0069/16 awarded for Faculty of Environmental Engineering Wrocław University of Science and Technology by Ministry of Science and Higher Education in years 2016–2017.

References

1. PN-EN 752:2008, *Drain and sewer systems outside buildings* (PKN, Warszawa, 2008)
2. Rozporządzenie Ministra Środowiska z dnia 18 listopada 2014 r., Dz. U. RP z dnia 16 grudnia 2014 r., poz. 1800

3. A. Kotowski, *Basics of safe dimensioning of drainage areas* (Seidel-Przywecki, Wrocław, 2015)
4. M. Nowakowska, *Identification of hydrological and hydraulic parameters of urban catchment area in SWMM hydrodynamic modeling* (Oficyna Wydawnicza Politechniki Wrocławskiej, Wrocław, 2016)
5. M. Nowakowska, A. Kotowski, *Methodology and rules for modelling drainage of urban areas* (Oficyna Wydawnicza Politechniki Wrocławskiej, Wrocław, 2017)
6. M. Mrowiec, *Effective dimensioning and dynamic regulation of sewerage retention tanks* (PCz., Częstochowa, 2009)
7. M. Skotnicki, M. Sowiński, *Verification of the method for determining the hydraulic width of a sub-catchment on the example of a selected urban catchment* (PW., Warszawa, 2009)
8. D. Słyś, A. Stec, *Environ. Prot. Eng.* **38**, 99–112 (2012)
9. M. Zawilski, G. Sakson, *Gaz, Woda Tech. Sanit.* **11**, 32–36 (2010)
10. M. Zawilski, G. Sakson, *Gaz, Woda Tech. Sanit.* **9**, 321–323 (2011)
11. M. Zawilski, *Gaz, Woda Tech. Sanit.* **6**, 28–32 (2010)
12. A. Kotowski, B. Kaźmierczak, A. Dancewicz, *Modeling precipitation for sewage dimensioning* (PAN, **68**, Warszawa, 2010)
13. I.R.A. Green, D. Stephenson, *Hydrologie Sciences J.* **31**, 395–411 (1986)
14. W. James, *Rules for responsible modeling* (CHI Publications, Guelph, 2003)
15. M. Ozga-Zielińska, J. Brzeziński, *Practical hydrology* (PWN, Warszawa, 1997)
16. ASCE, *Design & Construction of Urban Stormwater Management Systems* (New York 1992)
17. U.K. Maheepala, A.K. Takyi, B.J.C. Perera, *J. Hydrology* **245**, 32–47 (2001)
18. R. Mccuen, P. Johnson, R. Ragan, *Hydrology* (Federal Highway Administration, Washington, 1996)
19. PIT R., *Infiltration Through Disturbed Urban Soils and Compost-Amended Soil Effects on Runoff Quality and Quantity*. United States Environmental Protection Agency, Washington (1999)
20. L.A. Rossman, *Storm Water Management Model. User's Manual*. United States Environmental Protection Agency, Washington (2010)